










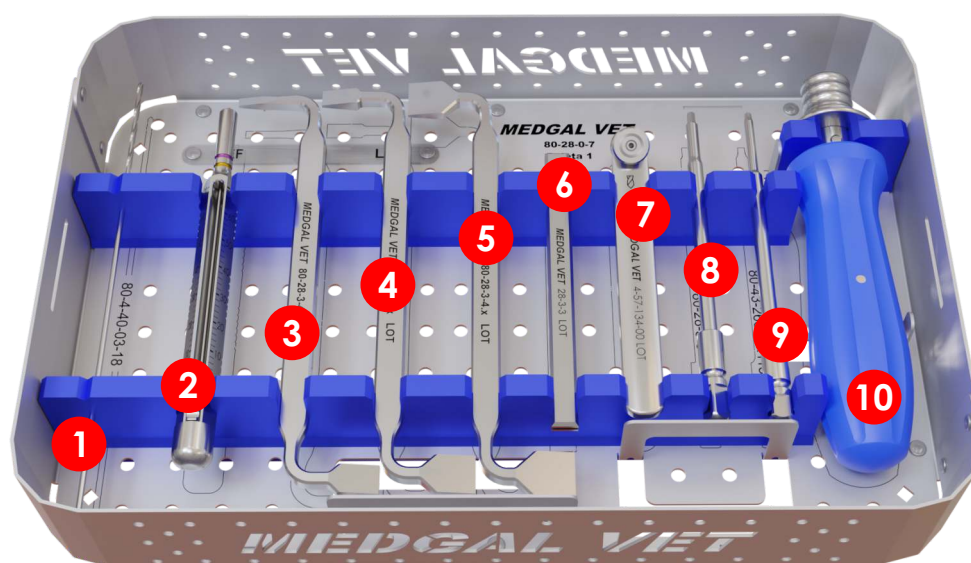

**INSTRUMENTARIUM DO KLATEK TTA-MI
80-28-0-7**



- | | | | |
|-----------|-------------------------|---------------------------------|--|
| 1 | 80-4-40-03-18 | Wiertła chirurgiczne Ø 1.8 |  |
| 2 | 80-57-307-0 | Miarka grubości kości |  |
| 3 | 80-28-3-4.3 | Rozszerzacz kostny 3/9 mm |  |
| 4 | 80-28-3-4.2 | Rozszerzacz kostny 6/12 mm |  |
| 5 | 80-28-3-4.1 | Rozszerzacz kostny 13,5/15 mm |  |
| 6 | 80-28-3-3 | Giętak do uszek |  |
| 7 | 80-4-57-134-00 | Prowadnik wiertła Ø 1.8 |  |
| 8 | 80-28-5-3 | Trzpień S2.5 |  |
| 9 | 80-43-268-T8.115 | Trzpień TORX T8 |  |
| 10 | 80-28-5-1 | Rękojeść do wymiennych trzpieni |  |